MK2866 HPLC

Client	:SARMS4LESS
Test time	:05/08/2021
Product Name	:MK2866
Analyst	:GSL
Lot No.	:20210508
Column:	:GSA46250BIO17013,C18, 4.6*250mm,5um
Solvent A	:100% Acetonitrile
Solvent B	:0.1% Trifluoroacetic in 100% Water
Gradient	:

	A	B
0.0min	5%	95%
20.0min	95%	5%
20.1min	100%	0%
30.0min	Stop	

Flow Rate	:1.0ml/min
Wavelength	:220nm
Temperature	:40℃
Concentration	:1mg/ml
Sample Volume	:6ul

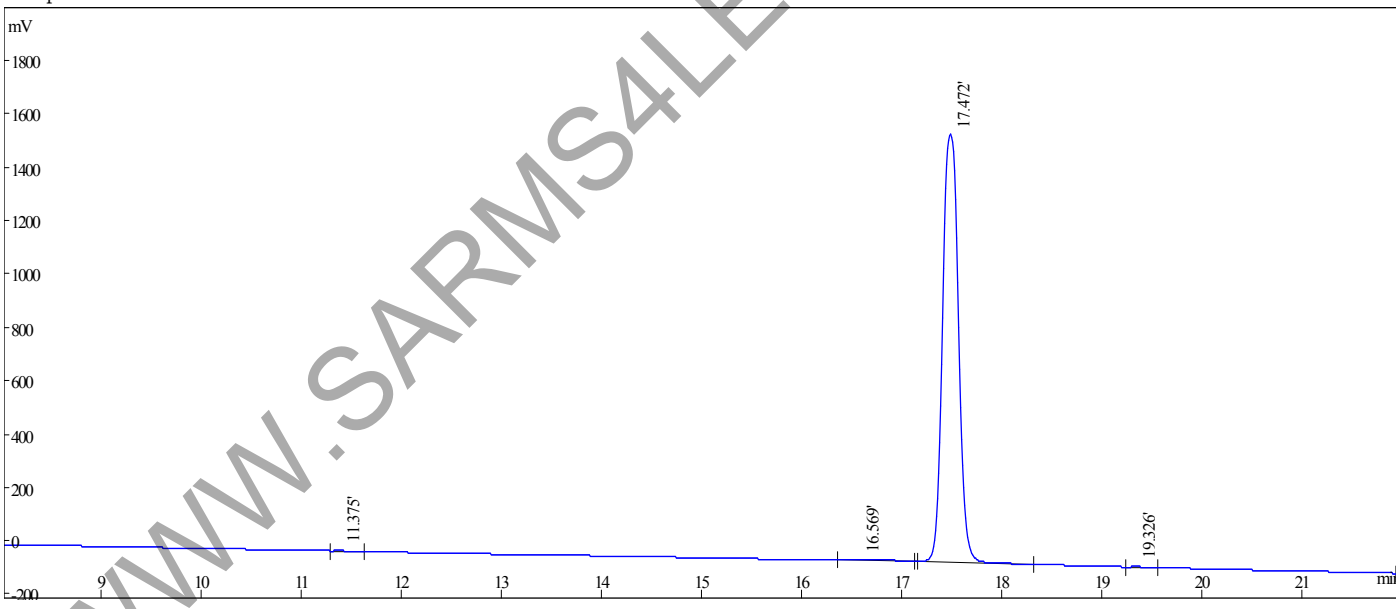

No.	Stay time	Concentration	Peak area	Peak height
1	11.375	0.04511	8116	901
2	16.569	0.1918	34511	1181
3	17.472	98.65	17747814	1602343
4	19.326	0.07426	13360	1619
5	22.183	1.046	188198	4463
Total		100	17991999	1610507

WWW.SARMS4LESS.COM