


S4 HPLC

Client : SARMS4LESS
 Test time : 05/10/2021
 Product Name : S4
 Analyst : LJ
 Lot No. : 20210510
 Column: : GSA46250BI017013, C18, 4.6*250mm, 5um
 Solvent A : 100% Acetonitrile
 Solvent B : 0.1% Trifluoroacetic in 100% Water
 Gradient :
 A B
 0.0min 40% 60%
 25.0min 60% 40%
 25.1min 100% 0%
 30.0min Stop
 Flow Rate : 1.0ml/min
 Wavelength : 220nm
 Temperature : 37°C
 Concentration : 1mg/ml
 Sample Volume : 10ul

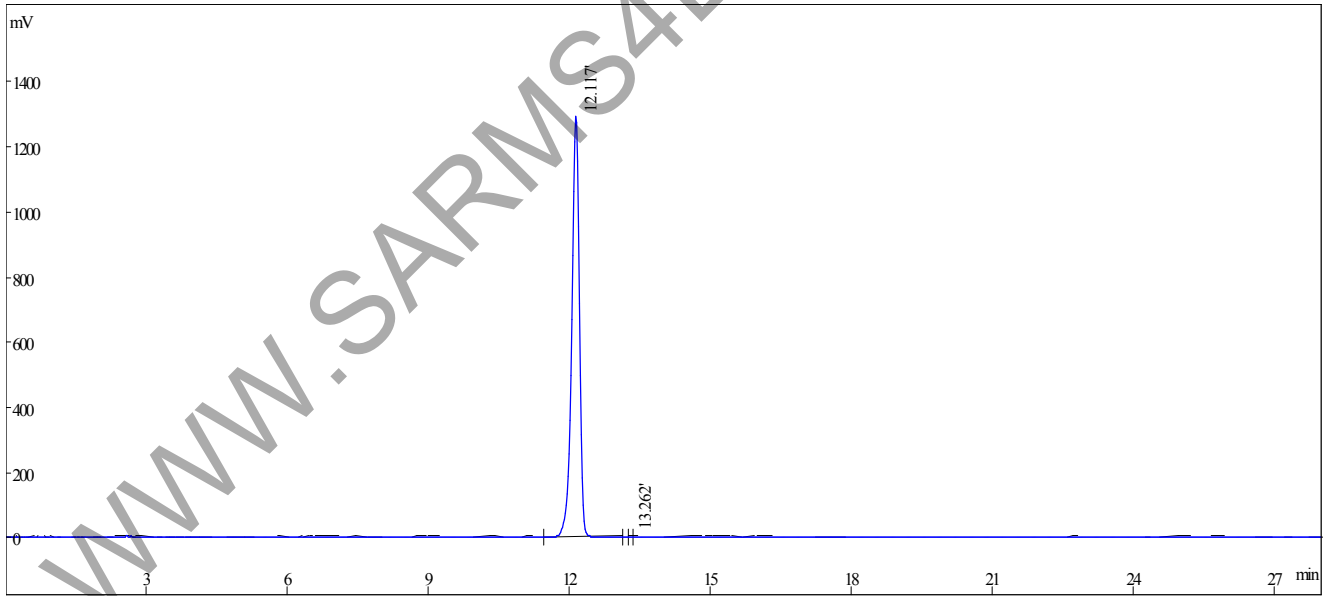

Number	Stay time	Concentration	Peak area	Peak height
1	12.117	99.9	14787445	1304725
2	13.262	0.0004162	62	22
Total		100	14787507	1304747